


## PE anti-human CD4 Antibody

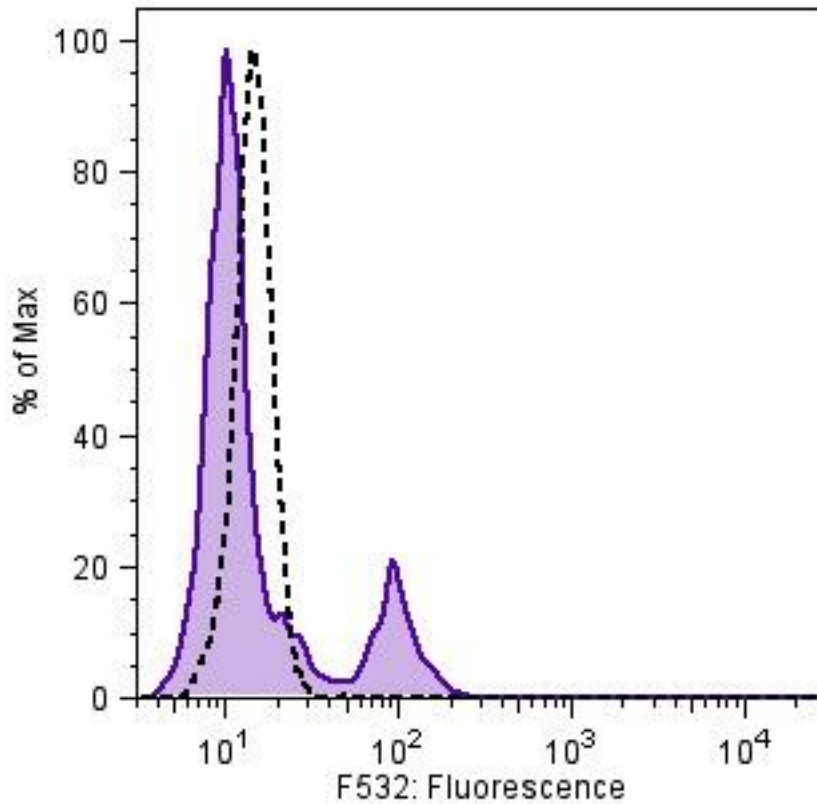

Human peripheral blood was stained with CD4 (clone RPA-T4) PE (solid line) or mouse IgG1,  $\kappa$  PE isotype control (dashed line).

Data was acquired on the Moxi Flow, exported, and processed using FlowJo software.